

Figure S1A- Trainees in the practical session



Figure S1B-Bleb visible at the sausage surface, after injection of 0.1 mL of saline



Figure S2: Schematic of training and evaluation process (icons by Freepik)

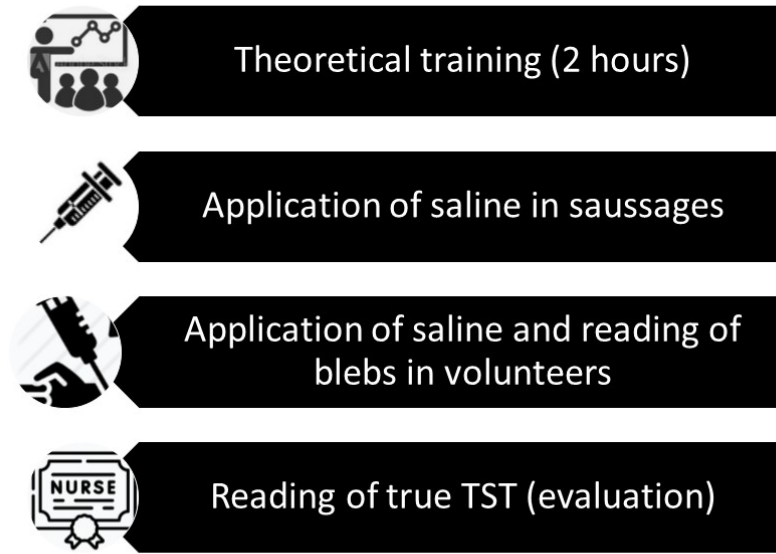


Figure S3 Caliper ruler for TST reading used in training and evaluation sessions.

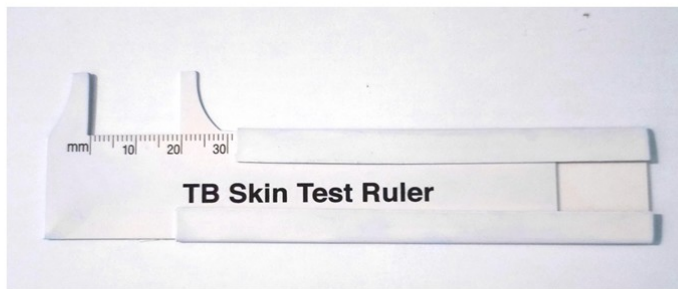


Table-S1 Percentage of agreement of the readings of trainees with trainer, stratified by the tuberculin skin test results

Trainer	0-4 mm n (%)	5-9 mm n (%)	≥10 mm n (%)	Total n (%)
Trainees				
1	6 (30)	1 (5)	6 (30)	20 (65)
2	6 (37)	0 (0)	7 (44)	16 (81)
3	2 (67)	0 (0)	1 (33)	3 (100)
4	3 (75)	0 (0)	0 (0)	4 (75)
5	0 (0)	1 (14)	1 (14)	7 (28)
6	0 (0)	0 (0)	2 (67)	3 (67)
7	1 (12)	1 (12)	6 (75)	8 (100)
8	1 (14)	2 (29)	1 (14)	7 (57)
9	1 (14)	1 (14)	2 (29)	7 (57)
10	0 (0)	1 (25)	3 (75)	4 (100)
11	1 (11)	2 (22)	4 (44)	9 (78)
Mean percentage (± standard deviation)	24 (± 26)	11 (± 11)	39 (± 25)	73 (±22)